

# Sequencing Quality Control Report

Genomics Unit

April 18, 2015

## 1 Flowcell Information



Flowcell AC6DTUANXX  
Run Start 2015-04-15  
Read Length 50 paired end  
HiSeq Sequencing Kit TruSeq v4

Sequencer Software HiSeq Control Software 2.2.58  
Gerald version 1.8


## 2 Samples Information

LabID	Name	Index	NumberOfReadPairs
7339	ATAC lib B	TAAGGC	135208520
7340	ATAC lib 18	CGTACT	150206888
7341	ATAC lib d1	AGGCAG	140250471
7342	ATAC lib d2	TCCTGA	122073470
7592	ATAC Lib E14	GGACTC	72475028
8188	GMP ATAC lib	TAGGCA	89471976


### 3 Quality Plots

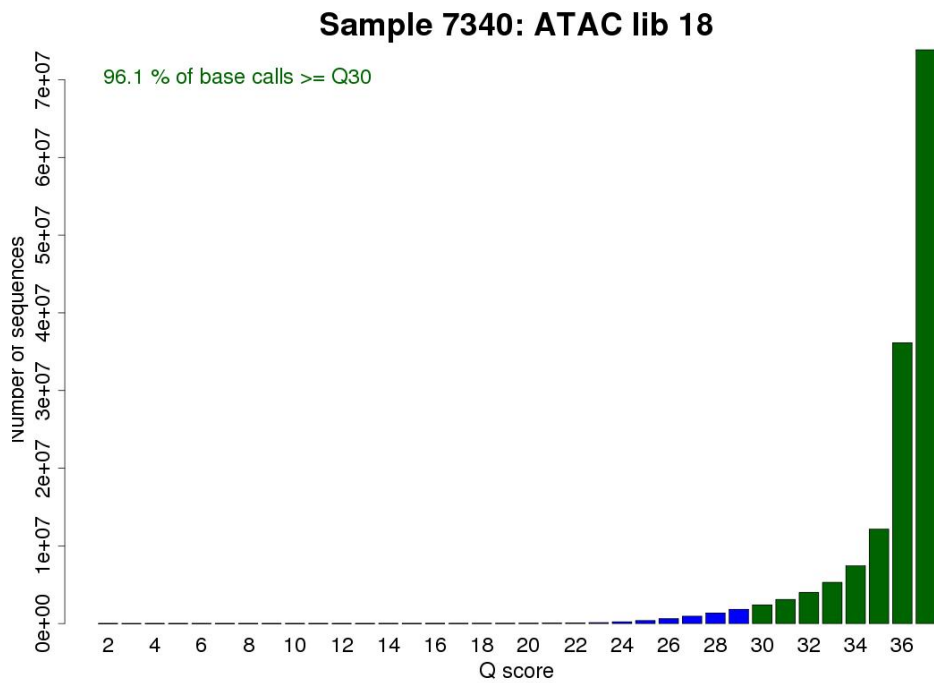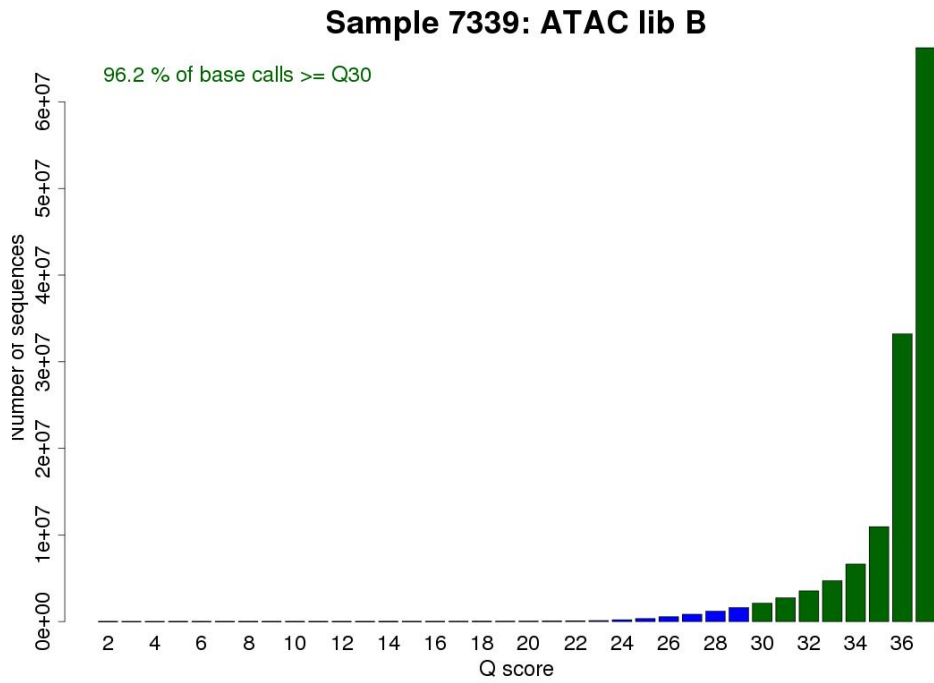


### Sample 7341: ATAC lib d1

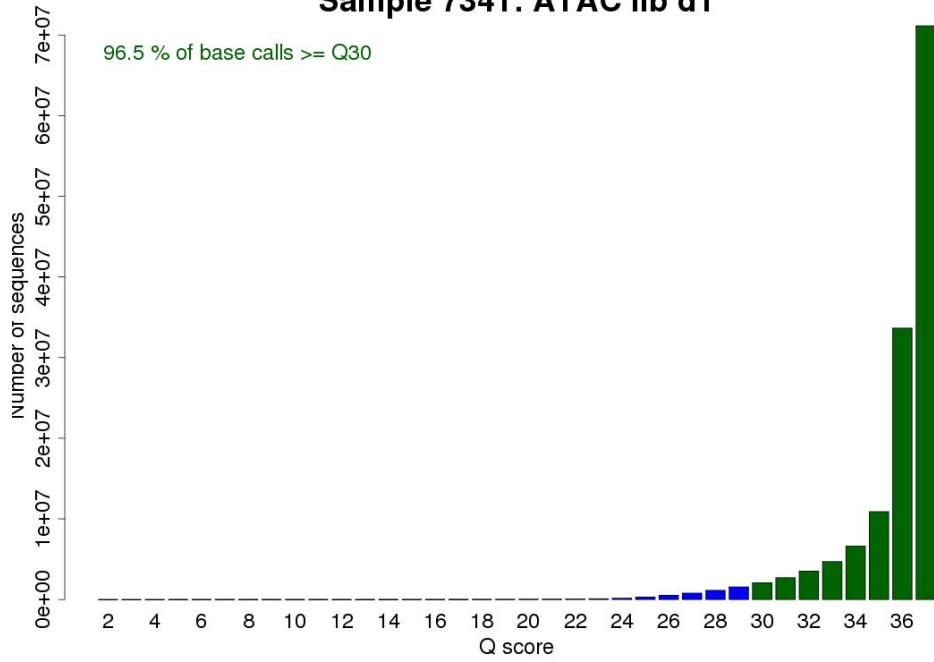

### Sample 7342: ATAC lib d2

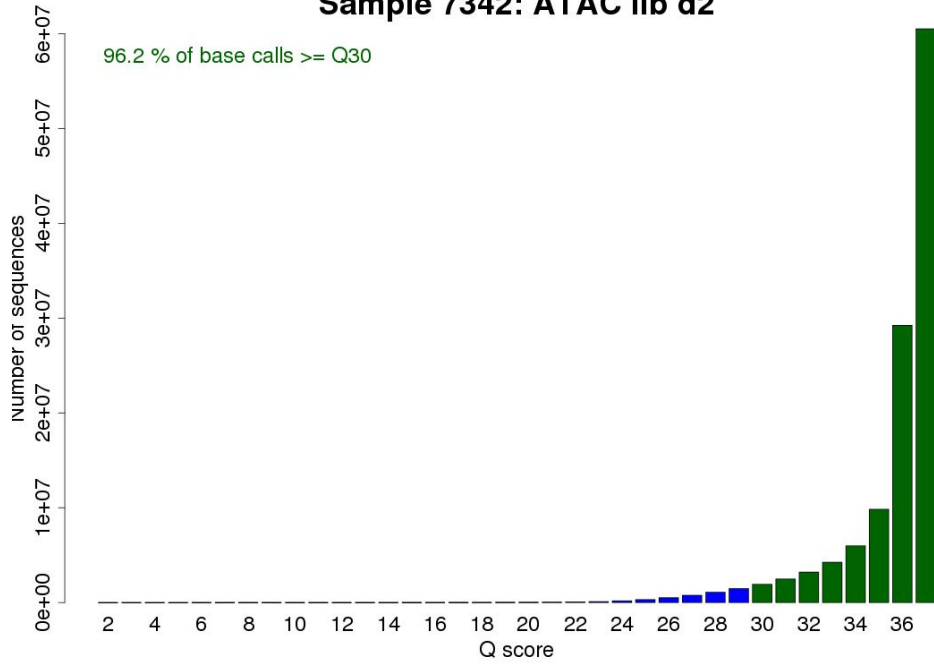

### Sample 7592: ATAC Lib E14

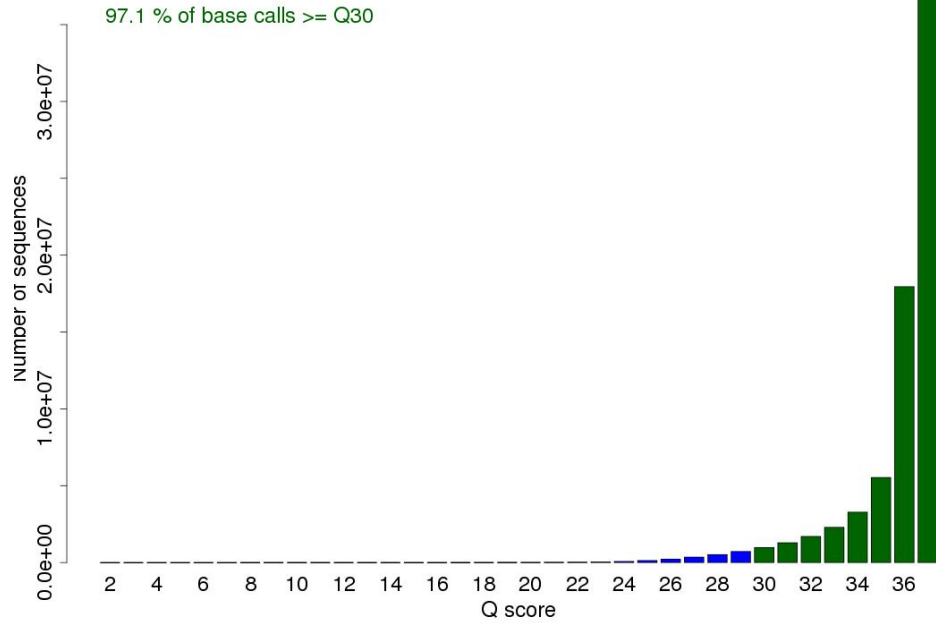

### Sample 8188: GMP ATAC lib

